

ERROR CODES QUICK TROUBLESHOOTING GUIDE

<p>X51</p>		<p>'Please close the cover'</p> <p>For safety the unit will not run with the lid open. Please close the cover when you are ready to start.</p>
<p>X41</p>		<p>'Liquitab beaker missing or in wrong position'</p> <p>Please ensure a new myLiquitab beaker is in the unit and that it is sitting in the correctly aligned position.</p>
<p>X21</p>		<p>'Overheat - Auto Rest for 20 mins'</p> <p>The unit has overheated and has gone into auto rest mode. The unit will turn back on once it is sufficiently cool.</p>
<p>X31</p>	<p>ERROR CODE: X31 Temperature sensor error.</p>	<p>'Temperature Sensor Error'</p> <p>The unit must be returned for repair. Please contact service@myliquitab.com or visit www.myliquitab.com/service</p>
<p>X11</p>	<p>Temperature warning mark</p> 	<p>'°C'</p> <p>The unit is running outside its temperature parameters. Allow the unit some time to cool before re-using.</p>

'Change water'
Periodically a message will appear to remind the user to change the water in the reservoir. If it has been changed the message can be deleted.

CLEANING AND MAINTENANCE

- 1) It is recommended that the stirring paddle (on the underside of the lid on the myLiquitab Homecare Unit) be cleaned after each use. A Stirring Paddle is provided in the Homecare Pack which also includes myLiquitab Beakers.
- 2) It is recommended that the underside of the lid be thoroughly wiped after each use.
- 3) It is recommended that the reservoir water should be emptied after each use. The myLiquitab Unit should not be run without water in the reservoir.

USE OF MYLIQUITAB BEAKERS

myLiquitab Beaker use in the Home Setting.

Each myLiquitab Beaker can be used 3-4 times by a single user. To minimise the potential risk of cross contamination please ensure that the beaker is washed and dried thoroughly between each use.

myLiquitab recommends that each beaker is used **ONCE ONLY** to minimise the risk of cross contamination and to ensure you get 'your medication only.'

myLiquitab Beaker use in the Clinical Setting.

The myLiquitab Unit can be used in a clinical setting for up to 6 people, each with 6 serves per day. Each myLiquitab Beaker is to be used **ONCE ONLY** to ensure clinical outcomes against cross infection and cross contamination.

myLiquitab Beakers are 100% recyclable.

This appliance is not intended for use by persons (including children) with reduced physical, sensory or mental capabilities, or lack of experience and knowledge, unless they have been given supervision or instruction concerning use of the appliance by a person responsible for their safety. Children should be supervised to ensure that they do not play with the appliance.

Enteric coated, sustained release and slow release tablets should not be liquefied in a myLiquitab Homecare Unit. It is advisable that you speak with your doctor and/or pharmacist regarding which medications can or can't be used in a myLiquitab Homecare Unit.

For service enquiries about the myLiquitab Homecare Unit please email service@myliquitab.com or visit www.myliquitab.com/service

myliquitab[®]
homecare

For information email
info@myliquitab.com
www.myliquitab.com

myLiquitab and Liquitab are registered or Common Law trade marks of Liquitab Systems Limited. Liquitab Systems Limited has patents or patents applications in a number of countries. Liquitab Systems Limited reserves the right to alter product specifications without notice as a result of our ongoing policy of product improvement. © 2018 myLiquitab. All rights reserved. Made in China.

LIQ 08058

Instructions for use and care of the myLiquitab Homecare Unit.




www.myliquitab.com

myliquitab[®]
homecare

Thank you for purchasing a myLiquitab Homecare Unit. Please read and follow the instructions below to ensure the correct use and care of the unit.

CAUTION

- 1) Please read these instructions carefully.
- 2) Enteric coated, sustained release and slow release tablets should not be liquefied in a myLiquitab Homecare Unit. It is advisable that you speak with your doctor and/or pharmacist regarding which medications can or can't be used in a myLiquitab Homecare Unit.
- 4) The myLiquitab Homecare Unit has been designed for use in the home. For high frequency or institutional use, please contact myLiquitab.
- 5) Use only a myLiquitab Beaker in a myLiquitab Homecare Unit.

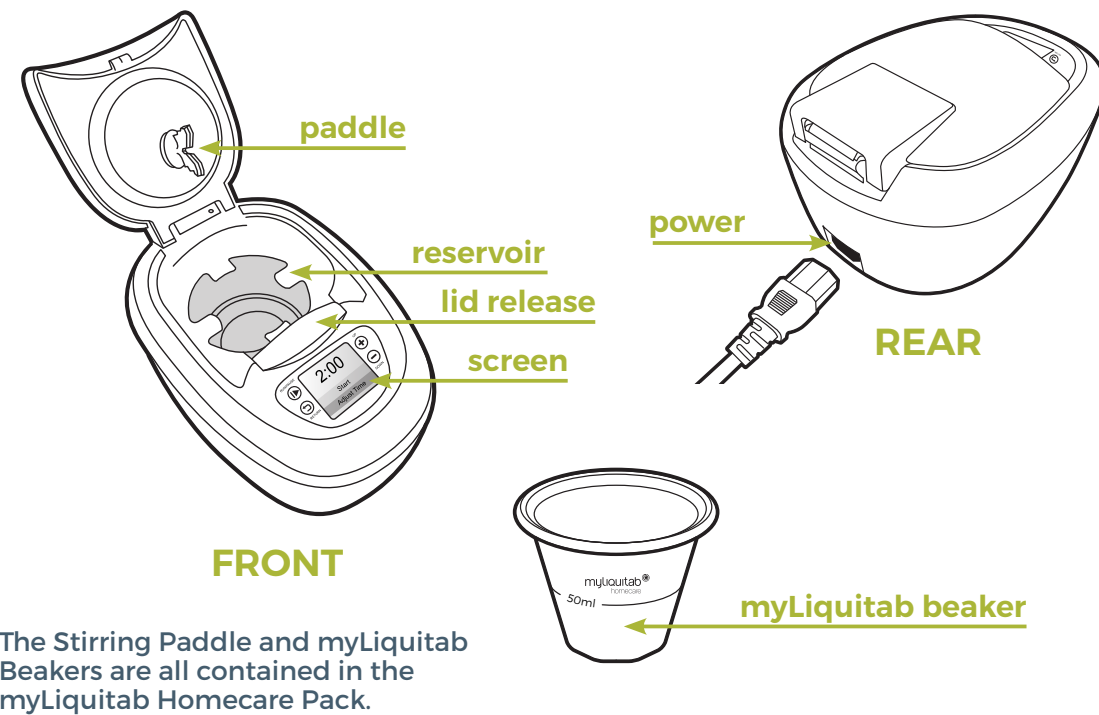

SET UP

- 1) Please remove the myLiquitab Homecare Unit from its box and packaging.
- 2) Plug in the electrical power cable into the socket at the rear of the myLiquitab Homecare Unit.
- 3) Fit the stirring paddle (contained in the Homecare Pack) to the underside of the myLiquitab Unit's lid.

USE

<p>1</p> <p>Open the lid of the myLiquitab Homecare Unit by pressing the silver release button.</p>	<p>2</p> <p>Add 50ml of clean water to the myLiquitab Unit's reservoir.</p> <p>NB: The reservoir water should be emptied after each use. The myLiquitab Unit should not be run without water in the reservoir.</p>
<p>3</p> <p>Fill the myLiquitab beaker with water to the indicator line. Add your tablet(s) and 1 scoop (6gm) of myLiquitab flavouring.</p> <p>NB: It is recommended that myLiquitab flavouring be used as it has been designed for use in the myLiquitab Homecare Unit</p> <p>If your tablets are large, please break them in half.</p>	<p>4</p> <p>Place the myLiquitab beaker upright in the myLiquitab Homecare Unit and close the myLiquitab Homecare Unit's lid.</p>
<p>5</p> <p>Press the Run/Pause button. The myLiquitab Homecare Unit is pre-programmed to run for 2 minutes. This time can be increased or decreased depending on the size and number of tablets to be liquefied. To adjust the time, use the Up [+] and Down [-] Buttons on the Unit.</p>	
<p>6</p> <p>When the cycle is complete the Unit will stop and sound a 'beep.' Open the myLiquitab Homecare Unit by pressing the silver button to release the lid.</p> <p>It is recommended a spoon is used to check the tablets have been fully dispersed in the liquid, if not place the beaker back into the Unit and repeat the cycle [from step 4].</p> <p>Hint: For future use the cycle time can be increased, [based on the same dose] if more than 1 cycle was required previously. The time can be set to the combined time of the previous individual cycles.</p>	<p>7</p> <p>Please check that the medication has been fully dispersed into the liquid. It is advisable that the liquid is checked with a spoon prior to consuming to ensure no larger particles remain. If particles remain please repeat step 5.</p> <p>NB: It is also recommended that the liquified medication is consumed as soon as possible after using the myLiquitab Homecare Unit.</p> <p>Your liquified medication is ready to drink, swirl the beaker to ensure all contents are consumed.</p>

HOW TO ADJUST THE TIME

<p>The myLiquitab Homecare Unit is pre set to a running time of 2:00 minutes. The time can be increased (up to 4 min) or decreased in 30-second increments.</p>	<p>To adjust the time, push the minus button to align the bar on the LCD screen over the text 'Adjust Time'</p>
<p>Lock the 'Adjust Time' mode by selecting the run/pause button.</p>	<p>Decrease the desired time by using the minus button.</p>
<p>Increase the desired time by using the plus button.</p>	<p>Once the desired time has been selected return the unit to the start mode by selecting the return button. The bar on the LCD screen should cover the word 'Start.'</p>
<p>The unit can be run in the new time by selecting the run/pause button. The unit may be paused while running using the run/pause button and the balance of the time will be maintained.</p>	<p>The 'Return' button may be selected when the unit is paused to return the timer to the full set time.</p>